

RFB00035/12.20/6.4 Dieses Dokument ist urheberrechtlich geschützt • This document is protected by copyright • Rosenberger Hochfrequenztechnik GmbH & Co. KG


Technical Data Sheet

RPC-1.85


Calibration Kit Plug

Rosenberger

08S30R-MSOS3

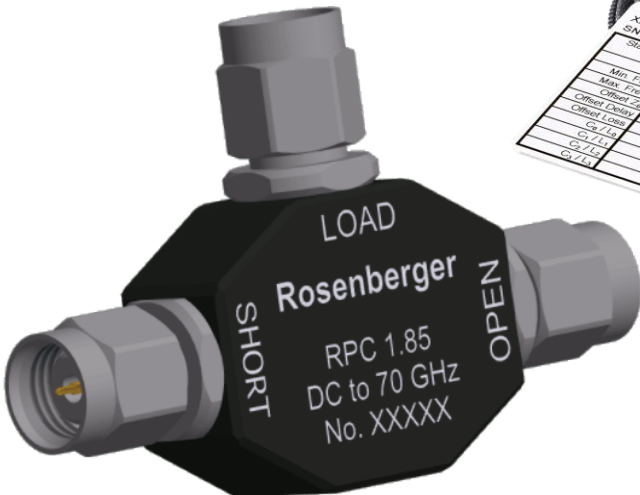

Calibration Kit			
SN XXXXX			
Standard	Thru (f.f.)	Load (f)	Open (f)
Min. Freq.	0	0	0
Max. Freq.	1.2	0	0
Offset Delay	50	50	50
Offset Loss	-200 dB	0	0
C ₁ / L ₁	2.5	0	0
C ₂ / L ₂	0	66.946	0
C ₃ / L ₃	0	0	9.94
C ₄ / L ₄	0	47.20	990.0
C ₅ / L ₅	0	990.0	112.50
C ₆ / L ₆	0	112.50	10.0

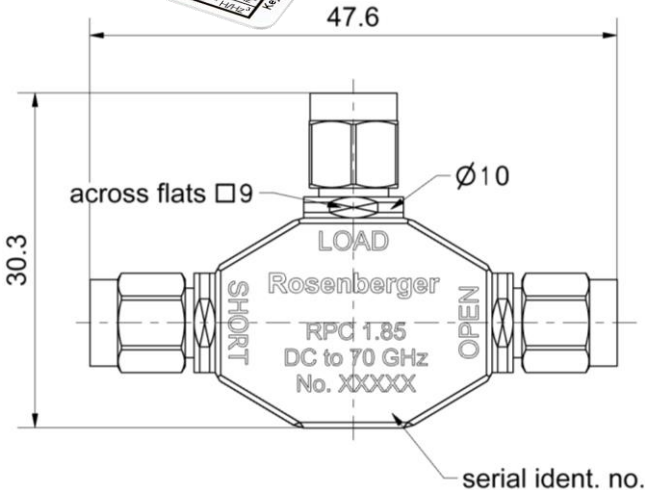

All dimensions are in mm; tolerances according to ISO 2768 m-H

Interface

According to
Mechanically compatible with

IEC 61169-32
RPC-2.40

Contents and Documentation

This kit is delivered with

- **Standard Definitions Card**
Printed Standard Definitions that can be used on nearly all Vector Network Analyzers
- **Certificate of Testing**
- **Hard Shell Case**
- **Protection Caps**
- **User Manual**

Material and plating

Connector parts

Center conductor
Outer conductor
Coupling nut
Body
Dielectric
Substrate

Material

CuBe
Stainless steel
Stainless steel
Aluminum
PS
Al₂O₃

Plating

Gold, min. 1.27 µm, over nickel
Passivated
Passivated
black anodized

Rosenberger Hochfrequenztechnik GmbH & Co. KG
P.O.Box 1260 D-84526 Tittmoning Germany
www.rosenberger.com

Tel. : +49 8684 18-0
Email : info@rosenberger.com

Page
1 / 3

Electrical data

Frequency range DC to 70.0 GHz

Open

Error from nominal phase¹

≤ 2.0°, DC to 4 GHz
≤ 5.0°, 4 GHz to 26.5 GHz
≤ 7.0°, 26.5 GHz to 50 GHz
≤ 10.0°, 50 GHz to 70 GHz

Short

Error from nominal phase²

≤ 2.0°, DC to 4 GHz
≤ 5.0°, 4 GHz to 26.5 GHz
≤ 7.0°, 26.5 GHz to 50 GHz
≤ 10.0°, 50 GHz to 70 GHz

Load

Return loss

≥ 35.0 dB, DC to 4 GHz
≥ 25.0 dB, 4 GHz to 26.5 GHz
≥ 22.0 dB, 26.5 GHz to 50 GHz
≥ 20.0 dB, 50 GHz to 70 GHz

DC Resistance

50 Ω ± 0.5 Ω

Power handling (at 25 °C, sea level)

≤ 0.5 W, derate by 0.005 W/K

¹ The nominal phase is defined by the Offset Delay, the Offset Loss and the Fringing Capacitances

² The nominal phase is defined by the Offset Delay, the Offset Loss and the Short Inductance

Mechanical data

Mating cycles	≥ 500
Maximum torque	1.65 Nm
Recommended torque	0.90 Nm
Gauge	0.00 mm to 0.03 mm

General standard definitions

For proper operation the vector network analyzer (VNA) needs a model describing the electrical behaviour of this calibration standard. The different models, units, and terms used will depend on the VNA type and they will have to be entered into the VNA. All values are based on typical geometry and plating.

Open

Offset Z ₀ / Impedance / Z ₀	50 Ω
Offset Delay	16.678 ps
Length (electrical) / Offset Length	5.00 mm
Offset Loss	3.75 GΩ/s
Loss	0.0109 dB/√GHz
Fringing Capacitances	$C_0 = 10.0000 \times 10^{-15} \text{ F} \quad / \quad 10.0000 \text{ fF}$ $C_1 = -500.000 \times 10^{-27} \text{ F/Hz} \quad / \quad -0.50000 \text{ fF /GHz}$ $C_2 = 11.5000 \times 10^{-36} \text{ F/Hz}^2 \quad / \quad 0.01150 \text{ fF /GHz}^2$ $C_3 = -0.10000 \times 10^{-45} \text{ F/Hz}^3 \quad / \quad -0.00010 \text{ fF /GHz}^3$

Technical Data Sheet				Rosenberger			
RPC-1.85		Calibration Kit Plug		08S30R-MSOS3			
Short Offset Z_o / Impedance / Z_o Offset Delay Length (electrical) / Offset Length Offset Loss Loss Short Inductance $50\ \Omega$ 16.678 ps 5.00 mm 4.17 GΩ/s 0.0121 dB/ $\sqrt{\text{GHz}}$ $L_0 = -12.0000 \times 10^{-12}\ \text{H}$ / -12.000 pH $L_1 = 250.000 \times 10^{-24}\ \text{H/Hz}$ / 0.25000 pH/GHz $L_2 = -8.10000 \times 10^{-33}\ \text{H/Hz}^2$ / -0.00810 pH/GHz² $L_3 = 0.08000 \times 10^{-42}\ \text{H/Hz}^3$ / 0.00008 pH/GHz³							
Load Offset Z_o / Impedance / Z_o Offset Delay Length (electrical) / Offset Length Offset Loss Loss $50\ \Omega$ 0.0000 ps 0.000 mm 0.00 GΩ/s 0.0000 dB/ $\sqrt{\text{GHz}}$							
Environmental data Operating temperature range³ Rated temperature range of use⁴ Storage temperature range RoHS + 20 °C to +26 °C 0 °C to +50 °C - 40 °C to +85 °C compliant							
³ Temperature range over which these specifications are valid. ⁴ This range is underneath and above the operating temperature range, within the calibration kit is fully functional and could be used without damage							
Declaration of documentation Standard delivery for this kit includes Test Results. The documentation issued reports which quantities were tested individually, traceable to national / international standards. Model based standard definitions of the calibration standards are reported in Agilent / Keysight, Rohde & Schwarz and Anritsu compatible VNA format.							
Inspection interval Recommendation 12 months							
Packing Weight 28 g/pce							
While the information has been carefully compiled to the best of our knowledge, nothing is intended as representation or warranty on our part and no statement herein shall be construed as recommendation to infringe existing patents. In the effort to improve our products, we reserve the right to make changes judged to be necessary. For the installation of the electrotechnical equipment, particular electrotechnical expertise is required. 							
Draft		Date		Approved		Date	
Marcel Panicke		12.04.18		Lars Ramtke		30.05.23	
Rev.		Engineering change number		Name		Date	
d00		23-0004		Marion Striegler		23.05.23	
Rosenberger Hochfrequenztechnik GmbH & Co. KG P.O.Box 1260 D-84526 Tittmoning Germany www.rosenberger.com						Tel. : +49 8684 18-0 Email : info@rosenberger.com	
						Page 3 / 3	